

# Research of Biological Effects of EM Field: Technical Equipment

*Jan Vrba<sup>1</sup>, Luca Vannucchi<sup>2</sup>, Peter Peschke<sup>3</sup>, Paolo Togni<sup>1</sup>, Lukáš Višek<sup>1</sup>*

<sup>1</sup> Czech Technical University in Prague, Dept. of EM Field, Technická 2, Prague, Czech Republic, [vrba@fel.cvut.cz](mailto:vrba@fel.cvut.cz)

<sup>2</sup> University of Pisa, Pisa, Italy + Institute of Microbiology, Czech Academy of Sciences, Prague, Czech Republic

<sup>3</sup> German Cancer Research Center, Im Neuenheimer Feld 280, D-69120 Heidelberg, Heidelberg, Germany

## Abstract

Research of interactions between EM Field and biological systems is of growing interests elsewhere. In the Czech Republic there are several groups working in this field, mainly in international co-operations. We will describe here basic technical equipment developed for five different research projects in the discussed area of interactions of EM field and biological systems.

## 1. Introduction

In present time research institutions in the Czech Republic run research focused on studies of interactions between EM field and biological systems. These institutions are technically supported by Dept. of EM Field of the Czech Technical University in Prague. In this contribution we would like to give more details about that projects and technical results dealing with developed exposition systems. Three of discussed projects (one in Germany and two in Czech Republic) represent research simulating of the microwave hyperthermia treatment. Other two projects are focused on simulation of exposition by mobile phones. In the modern view, cancer is intended as a complex illness, involving the cells that undergo to transformation, their environment, and the general responses at biochemical and biological levels induced in the host. Consequently, the anti-cancer treatment protocols need to be multi-modal to reach curative effects. Especially after the technical improvements achieved in the last 15 years by bio-medical engineering, microscopy devices, and molecular biology methods, the combinations of therapeutic procedures are growing in interest in basic and clinical research. The combination of applied biological research together to the physical sciences can offer important perspectives in anticancer therapy (e.g. different methodologies and technical devices for application of energies to pathological tissues). The modern bioengineering knowledge applied to traditional tools, as the microscopy, has largely renewed and expanded the fields of their applications (e.g.: *in vivo* imaging), pushing the interest for direct morpho-functional investigations of the biomedical problems.

## 2. Waveguide applicator

Very good results of EM field expositions applied on biological systems can be obtained by simple but efficient waveguide applicators, see example in Fig. 1.



Fig.1. Waveguide applicator for biological experiments.

Waveguide applicators offer a very big advantage – in approximately fifty percents of its aperture the irradiated electromagnetic field topology is very near to a plane wave, which is basic assumption for good homogeneity of the heating and optimal treatment penetration. Here described system is being used for research projects by two institutions (Institute of Radiation Oncology in Prague and Institute of Microbiology of the Czech Academy of Sciences). Aperture

of this waveguide is 48 x 24 mm and it is excited at frequency 2.45 GHz. Effective heating is in the middle of the real aperture – its size is approximately 24 x 24 mm. Waveguide is filled by teflon to reduce its cut-off frequency. Power from generator is possible to control from 10 to 180 W, in these experiments we worked between 10 and 20 W mostly.

### 3. Evaluation of waveguide applicator

To evaluate this applicator from technical point of view we made a series of experiments, see e.g. Fig. 2, where you can see example of measurement of temperature distribution by IR camera.

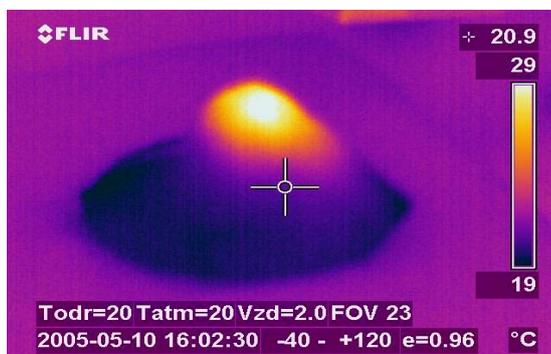


Fig.2. Temperature distribution obtained on surface of a model of mouse.

Here you can see temperature distribution obtained on surface of a model of mouse made from agar, with a simulated tumour on mouse back. Experiment has been done by heating of phantom during 2 minutes delivering a power of 10 W. Maximum of temperature increase has been found approximately 10 °C. Similar results with different increase in temperature we have got also in other technical experiments on phantom or live mouse when power or heating time was changed. Next figure gives example of temperature increase on the surface of the phantom and 1 cm in that phantom. Heating here is scheduled to 9 times repeated 30 s of heating and 30 s pause. Difference in temperature on the surface and under it is on the level of 1°C. That means very good homogeneity of temperature distribution in the treated area during planned biological experiments.

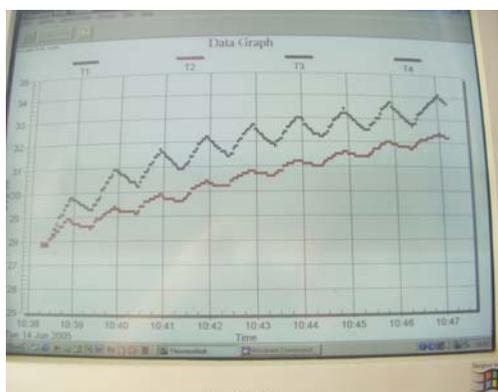


Fig. 3. Temperatures vs. time during experiments.

### 4. Array applicator

The main goal of the planned biological experiment is a simulation of a hyperthermia treatment of the experimentally induced pedicle tumours of the rat and to verify the feasibility of ultrasound diagnostics and magnetic resonance imaging respectively to map the temperature distribution in the target area of the treatment. Temperature to be reached is 41 °C or more (i.e. temperature increase of at least 4°C from starting point 37 °C), time period of heating is 45 minutes. Considering the necessary effective heating depth for the planned experiments, we have found 915 MHz to be suitable frequency. As an excellent compatibility of the applicator with non-invasive temperature measurement system (ultrasound or NMR) is a fundamental condition for our project, we should have to use non-magnetic metallic sheets of minimised dimensions to create the conductive elements of the applicator. Therefore the applicator itself (see Fig.4) is created by two inductive loops tuned to resonance by capacitive elements. Dimensions of these resonant loops

were designed by our software, developed for this purpose. Coupling between coaxial feeder and resonant loops (not shown in Fig.4) as well as a mutual coupling between resonating loops could be adjusted to optimum by microwave network analyser. The position of the loops is fixed by perspex holder. There is a special cylindrical space for experimental animal in lower part of this perspex holder. As the heated tissue has a high dielectric losses, both loops are very well separated and so no significant resonance in heated area can occur. From this follows, that either the position of the loops with respect to heated area or the distance between the loops is not very critical. First measurements to evaluate the basic properties of the discussed applicator were done on agar phantom of muscle tissue:

- evaluation of basic microwave properties (transfer of EM energy to the tissue, reflections),
- evaluation of compatibility with US and NMR,
- calculation and measurement of SAR and temperature distribution and its homogeneity.

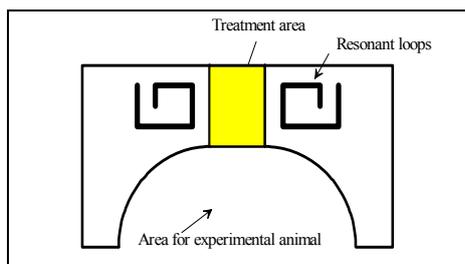


Figure 4. Arrangement of discussed microwave hyperthermia applicator.



Figure 5. Photograph of the discussed applicator

Exact tuning of the resonant loops to frequency 915 MHz has been easy and we could optimise the coupling between the coaxial feeder and resonant loops as well, with reflection coefficient less than 0.1. We have tested the power to be delivered to the applicator to obtain sufficient temperature increase (approximately 4 °C in less than 5 minutes is required). With power 10 W delivered to each loop for period of 2 minutes we succeeded to obtain the temperature increase of approximately 7 °C. To keep the increased temperature for a long time, 2 W in each loops were sufficient. Similar values were obtained during first experiments on rats also. Even with higher level of delivered microwave power we did not observe the change of resonant frequency (caused by increased temperature of the loops). This applicator has been developed for German Cancer Research Institute in Heidelberg. And it is being used there for a series of animal experiments to study effect of hyperthermia on tumours and possibility to combine hyperthermia with chemotherapy etc. Compatibility of this applicator with a Magnetic resonance unit (MR) has been studied and it has been demonstrated. We have tested the influence of the applicators on US diagnostics and NMR imaging and the result of this evaluation shows very good compatibility. Only a negligible deterioration of the US images have been observed when the incident power was kept under 100 W. Details about influence of microwave power on MR imaging are given in Fig. 6. We can see here a sequence of images of the discussed applicator made by MR unit for four different cases. First case (upper left) is image for the case without power excitation of the applicator. Second case (left down) a power of 10 W has been delivered to each loop. We can see quite clear configuration of the applicator set-up. Third case (upper right) gives situation when 20 W has been delivered to each loop. Slight noise but still quite a clear configuration of the applicator set-up can be observed. Fourth case (right down) gives situation when 40 W has been delivered to each loop. In this case noise disturbed the possibility to observe the configuration of the applicator. In theoretical and experimental evaluation, the grade of homogeneity of the temperature distribution in the target area has been tested, see the Fig. 7. Our mathematical approach is based on idea of waveguide  $TM_{01}$  mode excited in the agar phantom under the given conditions (see the dashed lines). Very good agreement have been obtained when verifying these results numerically – see right side of the picture.

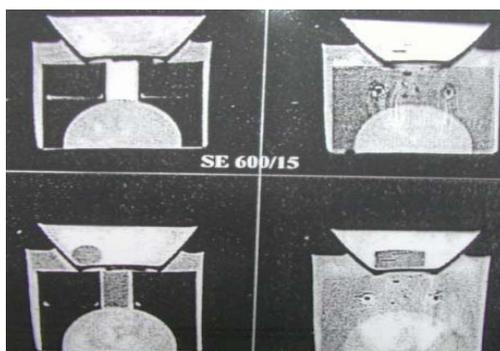


Fig. 6. MR images of the discussed applicator.

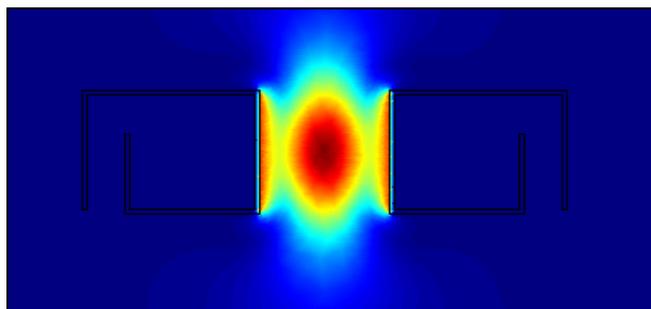


Fig. 7. SAR distribution (calculated by SEMCAD) in the heated agar phantom. Numerical SAR analysis.

Next figure shows experimental setup of applicator and simple exposure chambers installed at Medical Faculty of Charles University in Pilsen.



Fig. 10. Exposure system for research of EM field and biological system interactions.

## 5. Conclusions

In this paper we have described basic microwave technical equipment for biological experiments, i.e. waveguide applicator and so called array applicator, including its basic evaluations. As a novel results of our work we could mention that the new types of microwave applicator for basis biological research of cancer treatment and EM field interactions with biological systems have been developed and evaluated. Evaluation procedures have shown, that this applicator is a very effective heating structure and a compatibility with US and MR has been approved as well. Having approved these applicators in animal experiments, we are now working on development of their clinical versions to be used in clinical praxis soon.

## 6. Acknowledgements

This work was supported by the Czech Academy of Sciences, Institutional Research Concepts No. AV0Z50200510: “Hyperthermia and anticancer immunomodulation, morpho-functional study of micro-environmental interactions in melanoma model”.